

# MPR SERIES

32332628  
Issue K

## MicroPressure Board Mount Pressure Sensors Compact, High Accuracy, Compensated/Amplified

### DESCRIPTION

The MPR Series is a very small piezoresistive silicon pressure sensor offering a digital output for reading pressure over the specified full scale pressure span and temperature range. It is calibrated and compensated over a specific temperature range for sensor offset, sensitivity, temperature effects, and non-linearity using an on-board Application Specific Integrated Circuit (ASIC). This product is designed to meet the requirements of higher volume medical (consumer and non-consumer) devices, commercial appliance, and industrial/HVAC applications.

### DIFFERENTIATION

- Application-specific design addresses various application needs and challenges.
- Digital output: Plug and play feature enables ease of implementation and system level connectivity.
- Total Error Band: Provides a more comprehensive measurement of performance over the compensated temperature range, which minimizes testing and calibrating every sensor, thereby potentially reducing manufacturing cost; improves sensor accuracy and offers ease of sensor interchangeability due to minimal part-to-part variation. (See Figure 1.)


### VALUE TO CUSTOMERS

- Very small form factor: Enables portability by addressing weight, size, and space restrictions; occupies less area on the PCB.
- Wide pressure ranges simplify use.
- Enhances performance: Output accelerates performance through reduced conversion requirements and direct interface to microprocessors.
- Value solution: Cost-effective, higher volume solution with configurable options.

- Meets IPC/JEDEC J-STD-020D.1 Moisture Sensitivity Level 1 requirements: Allows avoidance of thermal and mechanical damage during solder reflow attachment and/or repair that lesser rated sensors may incur; allows long floor life when stored as specified (simplifying storage and reducing scrap); eliminates lengthy bakes prior to reflow, and allows for lean manufacturing due to stability and usability shortly after reflow.
- Meets food safety certification for North America, Europe and Asia (see Table 2).

### POTENTIAL APPLICATIONS

- **Consumer medical:** Non-invasive blood pressure monitoring, negative-pressure wound therapy, breast pumps, mobile oxygen concentrators, airflow monitors, CPAP water tanks, and medical wearables
- **Non-consumer medical:** Invasive blood pressure monitors, ambulatory blood pressure measurement, urine analyzers
- **Industrial:** Air braking systems, gas and water meters, natural gas metering, process gas monitoring, gas burner control, air compressors, gray water tank level measurement
- **Consumer:** Coffee machines, humidifiers, air beds, washing machines, dishwashers
- **Transportation:** CNG level monitoring, fuel level measurement



### FEATURES

- 5 mm x 5 mm [0.20 in x 0.20 in] package footprint
- Calibrated and compensated
- 60 mbar to 2.5 bar | 6 kPa to 250 kPa | 1 psi to 30 psi
- 24-bit digital I<sup>2</sup>C or SPI-compatible output
- IoT (Internet of Things) ready interface
- Stainless steel pressure port
- Compatible with a variety of liquid media
- Absolute and gage pressure types
- Total Error Band after customer auto-zero: As low as  $\pm 1.25$  %FSS
- Compensated temperature range: 0°C to 50°C [32°F to 122°F]
- REACH and RoHS compliant
- Meets IPC/JEDEC J-STD-020D.1 Moisture Sensitivity Level 1
- Select sensors available on breakout board for easy evaluation and testing
- Ultra-low power consumption (as low as 0.01 mW typ. average power, 1 Hz measurement frequency)
- Sensor materials have been tested and certified for these food safety standards: BPA Free, LFGB, NSF-169

### PORTFOLIO



The MPR Series joins an extensive line of board mount pressure sensors for potential use in medical, industrial, and consumer applications. To view the entire product portfolio, [click here](#).

**Honeywell**

# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS

## MPR SERIES

### Table of Contents

|   |             |
|---|-------------|
| <b>General Specifications</b> .....   | <b>3-4</b>  |
| <b>Power Consumption and Standby Mode</b> .....                               | <b>5-6</b>  |
| <b>Product Nomenclature and Order Guide</b> .....                             | <b>7</b>    |
| <b>Pressure Range Specifications:</b>   |             |
| 60 mbar to 2.5 bar .....  | 8           |
| 6 kPa to 250 kPa .....  | 9           |
| 1 psi to 30 psi .....   | 10          |
| 0 mmHg to 300 mmHg .....  | 10          |
| <b>1.0 GENERAL INFORMATION</b> .....  | <b>11</b>   |
| <b>2.0 PINOUT AND FUNCTIONALITY</b> .....                                     | <b>11</b>   |
| <b>3.0 START-UP TIMING</b> .....  | <b>11</b>   |
| <b>4.0 POWER SUPPLY REQUIREMENT</b> .....                                     | <b>11</b>   |
| <b>5.0 REFERENCE CIRCUIT DESIGN</b> .....                                     | <b>12</b>   |
| 5.1 I <sup>2</sup> C and SPI Circuit Diagrams .....                           | 12          |
| 5.2 Bypass Capacitor Use .....  | 12          |
| <b>6.0 I<sup>2</sup>C COMMUNICATIONS</b>                                      |             |
| 6.1 I <sup>2</sup> C Bus Configuration .....                                  | 13          |
| 6.2 I <sup>2</sup> C Data Transfer .....                                      | 13          |
| 6.3 I <sup>2</sup> C Sensor Address .....                                     | 13          |
| 6.4 I <sup>2</sup> C Pressure Reading .....                                   | 14          |
| 6.5 I <sup>2</sup> C Status Byte .....  | 14          |
| 6.6 I <sup>2</sup> C Communications .....                                     | 14          |
| 6.6.1 Output Measurement Command .....  | 14          |
| 6.6.2 I <sup>2</sup> C Sensor Address of 0x18 .....                           | 15          |
| 6.7 I <sup>2</sup> C Timing and Level Parameters .....                        | 15          |
| 6.8 Reference Code (Arduino/Genuino Uno) for I <sup>2</sup> C Interface ..... | 16          |
| <b>7.0 SPI COMMUNICATIONS</b>   |             |
| 7.1 SPI Definition .....  | 17          |
| 7.2 SPI Data Transfer .....   | 17          |
| 7.3 SPI Pressure Reading .....  | 17          |
| 7.4 SPI Status Byte .....   | 18          |
| 7.5 SPI Communications .....  | 18          |
| 7.6 SPI Timing and Level Parameters .....                                     | 18          |
| 7.7 Reference Code (Arduino/Genuino Uno) for SPI Interface .....              | 19          |
| <b>8.0 MPR SERIES DIGITAL OUTPUT PRESSURE CALCULATION</b> .....               | <b>20</b>   |
| <b>Long Port Dimensions and Recommended PCB Pad Layout</b> .....              | <b>21</b>   |
| <b>Short Port Dimensions and Recommended PCB Pad Layout</b> .....             | <b>22</b>   |
| <b>Tape and Reel Dimensions</b> .....   | <b>23</b>   |
| <b>Reflowable Protective Silicone Cap</b> .....                               | <b>24</b>   |
| <b>Reflowable Protective Silicone Cap Removal</b> .....                       | <b>24</b>   |
| <b>Recommended Tubing</b> .....   | <b>24</b>   |
| <b>Recommended O-Rings</b> .....  | <b>25</b>   |
| <b>Additional Information</b> .....   | <b>back</b> |


# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

**FIGURE 1. TEB COMPONENTS FOR THE MPR SERIES**

Total Error Band (TEB) is a single specification that includes the major sources of sensor error. TEB should not be confused with accuracy, which is actually a component of TEB. TEB is the worst error that the sensor could experience.

Honeywell uses the TEB specification in its datasheet because it is the most comprehensive measurement of a sensor’s true accuracy. Honeywell also provides the accuracy specification in order to provide a common comparison with competitors’ literature that does not use the TEB specification.

Many competitors do not use TEB—they simply specify the accuracy of their device. Their accuracy specification, however, may exclude certain parameters. On their datasheet, the errors are listed individually. When combined, the total error (or what would be TEB) could be significant.



**TABLE 1. ABSOLUTE MAXIMUM RATINGS<sup>1</sup>**

| Characteristic                             | Minimum                    | Maximum                   | Unit    |
|--|----------------------------|---------------------------|---------|
| Supply voltage ( $V_{\text{supply}}$ )     | -0.3                       | 3.6                       | Vdc     |
| Voltage on any pin                         | -0.3                       | $V_{\text{supply}} + 0.3$ | V       |
| ESD susceptibility (human body model)      | —                          | 4                         | kV      |
| Storage temperature                        | -40 [-40]                  | 85 [185]                  | °C [°F] |
| Soldering peak reflow temperature and time | 15 s max. at 250°C [482°F] |                           |         |

<sup>1</sup>Absolute maximum ratings are the extreme limits the device will withstand without damage.

**TABLE 2. ENVIRONMENTAL SPECIFICATIONS**

| Characteristic                                      | Parameter  |
|---|--|
| Humidity:<br>external surfaces<br>internal surfaces | 0 %RH to 95 %RH, non-condensing<br>0 %RH to 100 %RH, condensing  |
| Vibration   | 10 g, 10 Hz to 2 kHz   |
| Shock   | 50 g, 6 ms duration  |
| Solder reflow                                       | J-STD-020-D.1 Moisture Sensitivity Level 1 (unlimited shelf life when stored at $\leq 30^\circ\text{C}/85\% \text{RH}$ ) |
| Certification (food grade gel coating option)       | NSF-169, BPA Free, LFGB  |

**TABLE 3. WETTED MATERIALS**

| Component             | Material                                |
|-----------------------|---|
| Port                  | 304 stainless steel                     |
| Adhesives             | epoxy, silicone gel, fluorosilicone gel |
| Electronic components | silicon, glass, gold, aluminum          |
| Metal gel ring        | 304 stainless steel                     |

# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS

## MPR SERIES

**TABLE 4. SENSOR PRESSURE TYPES**

| Pressure Type | Description   |
|---------------|---|
| Absolute      | Output is proportional to the difference between applied pressure and a built-in vacuum reference.    |
| Gage          | Output is proportional to the difference between applied pressure and atmospheric (ambient) pressure. |

**TABLE 5. OPERATING SPECIFICATIONS**

| Characteristic                                       | Minimum   | Typical | Maximum  | Unit                   |
|--|-----------|---------|----------|------------------------|
| Supply voltage ( $V_{\text{supply}}$ ): <sup>1</sup> | 1.8       | 3.3     | 3.6      | Vdc                    |
| Current consumption:                                 |           |         |          |                        |
| I <sup>2</sup> C sleep/standby mode                  | 3.0       | 33.8    | 211      | nA                     |
| SPI sleep/standby mode                               | 13.0      | 43.8    | 221.0    | nA                     |
| Power consumption                                    | —         | 10      | —        | mW                     |
| Operating temperature range <sup>2</sup>             | -40 [-40] | —       | 85 [185] | °C [°F]                |
| Compensated temperature range <sup>3</sup>           | 0 [32]    | —       | 50 [122] | °C [°F]                |
| Startup time (power up to data ready)                | —         | —       | 2.5      | ms                     |
| Data rate (assumes command AA <sub>HEX</sub> )       | 161       | 204     | —        | samples per second     |
| I <sup>2</sup> C/SPI voltage level:                  |           |         |          |                        |
| low  | —         | —       | 20       | %V <sub>supply</sub>   |
| high   | 80        | —       | —        |                        |
| Pull up on MISO, SCLK, SS, MOSI                      | 1         | —       | —        | kOhm                   |
| Accuracy <sup>4</sup>                                | —         | —       | ±0.25    | %FSS BFSL <sup>5</sup> |
| Resolution:  |           |         |          |                        |
| transfer function A                                  | 14.0      | —       | —        | bits                   |
| transfer function B                                  | 13.5      | —       | —        |                        |
| transfer function C                                  | 14.0      | —       | —        |                        |

<sup>1</sup>The sensor is not reverse polarity protected. Incorrect application of supply voltage or ground to the wrong pin may cause electrical failure.

<sup>2</sup>**Operating temperature range:** The temperature range over which the sensor will produce an output proportional to pressure.

<sup>3</sup>**Compensated temperature range:** The temperature range over which the sensor will produce an output proportional to pressure within the specified performance limits (Total Error Band).

<sup>4</sup>**Accuracy:** The maximum deviation in output from a Best Fit Straight Line (BFSL) fitted to the output measured over the pressure range. Includes all errors due to pressure non-linearity, pressure hysteresis, and non-repeatability.

<sup>5</sup>**Full Scale Span (FSS):** The algebraic difference between the output signal measured at the maximum (Pmax.) and minimum (Pmin.) limits of the pressure range. (See Figure 4 for pressure ranges.)

# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES


## POWER CONSUMPTION AND STANDBY MODE

The sensor is normally in Standby Mode and is only turned on in response to a user command, thus minimizing power consumption. Upon receiving the user command, the sensor wakes up from Standby Mode, runs a measurement in Active State, and automatically returns to Standby Mode, awaiting the next command. The resulting sensor power consumption is a function of the sampling rate (samples per second) as shown in Tables 6 and 7 and Figures 2 and 3.

**TABLE 6. AVERAGE POWER CONSUMPTION AT 1.8 V<sub>SUPPLY</sub> (ASSUMES COMMAND AA<sub>HEX</sub>)**

| Sampling Rate (samples per second) | Average Power (mW) | Active Time (ms) | Active Power (mW) | Idle Time (ms) | Idle Power (mW) |
|------------------------------------|--------------------|------------------|-------------------|----------------|-----------------|
| <b>Minimum Average Power</b>       |                    |                  |                   |                |                 |
| 1                                  | 0.0068             | 3.625            | 1.884             | 996.375        | 0.0000054       |
| 2                                  | 0.0137             | 7.25             | 1.884             | 992.75         | 0.0000054       |
| 5                                  | 0.0341             | 18.125           | 1.884             | 981.875        | 0.0000054       |
| 10                                 | 0.0683             | 36.25            | 1.884             | 963.75         | 0.0000054       |
| 20                                 | 0.1366             | 72.5             | 1.884             | 963.75         | 0.0000054       |
| 50                                 | 0.3414             | 181.25           | 1.884             | 818.75         | 0.0000054       |
| 100                                | 0.6829             | 362.5            | 1.884             | 637.5          | 0.0000054       |
| 160                                | 1.0926             | 580              | 1.884             | 420            | 0.0000054       |
| <b>Typical Average Power</b>       |                    |                  |                   |                |                 |
| 1                                  | 0.0094             | 4.157            | 2.248             | 995.843        | 0.00006084      |
| 2                                  | 0.0187             | 8.314            | 2.248             | 991.686        | 0.00006084      |
| 5                                  | 0.0468             | 20.785           | 2.248             | 979.215        | 0.00006084      |
| 10                                 | 0.0935             | 41.57            | 2.248             | 958.43         | 0.00006084      |
| 20                                 | 0.1870             | 83.14            | 2.248             | 916.86         | 0.00006084      |
| 50                                 | 0.4673             | 207.85           | 2.248             | 792.15         | 0.00006084      |
| 100                                | 0.9345             | 415.7            | 2.248             | 584.3          | 0.00006084      |
| 160                                | 1.4592             | 665.12           | 2.248             | 334.88         | 0.00006084      |
| <b>Maximum Average Power</b>       |                    |                  |                   |                |                 |
| 1                                  | 0.0129             | 4.839            | 2.588             | 995.161        | 0.0003798       |
| 2                                  | 0.0254             | 9.678            | 2.588             | 990.322        | 0.0003798       |
| 5                                  | 0.0630             | 24.195           | 2.588             | 975.805        | 0.0003798       |
| 10                                 | 0.1256             | 48.39            | 2.588             | 951.61         | 0.0003798       |
| 20                                 | 0.2508             | 96.78            | 2.588             | 903.22         | 0.0003798       |
| 50                                 | 0.6264             | 241.95           | 2.588             | 758.05         | 0.0003798       |
| 100                                | 1.2524             | 483.9            | 2.588             | 516.1          | 0.0003798       |
| 160                                | 2.0036             | 774.24           | 2.588             | 225.76         | 0.0003798       |

**FIGURE 2. AVERAGE POWER CONSUMPTION VS SAMPLING RATE AT 1.8 V<sub>SUPPLY</sub>**




# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

**TABLE 7. AVERAGE POWER CONSUMPTION AT 3.3 V<sub>SUPPLY</sub> (ASSUMES COMMAND AA<sub>HEX</sub>)**

| Sampling Rate (Samples per second) | Average Power (mW) | Active Time (ms) | Active Power (mW) | Idle Time (ms) | Idle Power (mW) |
|------------------------------------|--------------------|------------------|-------------------|----------------|-----------------|
| <b>Minimum Average Power</b>       |                    |                  |                   |                |                 |
| 1                                  | 0.0114             | 3.625            | 3.134             | 996.375        | 0.0000099       |
| 2                                  | 0.0227             | 7.25             | 3.134             | 992.75         | 0.0000099       |
| 5                                  | 0.0568             | 18.125           | 3.134             | 981.875        | 0.0000099       |
| 10                                 | 0.1136             | 36.25            | 3.134             | 963.75         | 0.0000099       |
| 20                                 | 0.2272             | 72.5             | 3.134             | 963.75         | 0.0000099       |
| 50                                 | 0.5680             | 181.25           | 3.134             | 818.75         | 0.0000099       |
| 100                                | 1.1361             | 362.5            | 3.134             | 637.5          | 0.0000099       |
| 160                                | 1.8177             | 580              | 3.134             | 420            | 0.0000099       |
| <b>Typical Average Power</b>       |                    |                  |                   |                |                 |
| 1                                  | 0.0156             | 4.157            | 3.729             | 995.843        | 0.00011154      |
| 2                                  | 0.0311             | 8.314            | 3.729             | 991.686        | 0.00011154      |
| 5                                  | 0.0776             | 20.785           | 3.729             | 979.215        | 0.00011154      |
| 10                                 | 0.1551             | 41.57            | 3.729             | 958.43         | 0.00011154      |
| 20                                 | 0.3101             | 83.14            | 3.729             | 916.86         | 0.00011154      |
| 50                                 | 0.7751             | 207.85           | 3.729             | 792.15         | 0.00011154      |
| 100                                | 1.5501             | 415.7            | 3.729             | 584.3          | 0.00011154      |
| 160                                | 2.4800             | 665.12           | 3.729             | 334.88         | 0.00011154      |
| <b>Maximum Average Power</b>       |                    |                  |                   |                |                 |
| 1                                  | 0.0214             | 4.839            | 4.275             | 995.161        | 0.0006963       |
| 2                                  | 0.0421             | 9.678            | 4.275             | 990.322        | 0.0006963       |
| 5                                  | 0.1041             | 24.195           | 4.275             | 975.805        | 0.0006963       |
| 10                                 | 0.2075             | 48.39            | 4.275             | 951.61         | 0.0006963       |
| 20                                 | 0.4144             | 96.78            | 4.275             | 903.22         | 0.0006963       |
| 50                                 | 1.0349             | 241.95           | 4.275             | 758.05         | 0.0006963       |
| 100                                | 2.0692             | 483.9            | 4.275             | 516.1          | 0.0006963       |
| 160                                | 3.3103             | 774.24           | 4.275             | 225.76         | 0.0006963       |


**FIGURE 3. AVERAGE POWER CONSUMPTION VS SAMPLING RATE AT 3.3 V<sub>SUPPLY</sub>**



# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

FIGURE 4. PRODUCT NOMENCLATURE AND ORDER GUIDE

For example, **MPRLS0025PA00001A** defines an MPR Series pressure sensor, long port, silicone gel, 0 psi to 25 psi absolute pressure range, I<sup>2</sup>C, address 0x18, 10% to 90% of 2<sup>24</sup> counts transfer function, no breakout board.



### Pressure Range, Unit and Reference<sup>1</sup>


| Absolute      |                    | Absolute      |                  | Absolute      |                    | Gage                                      |                    |
|---------------|--------------------|---------------|------------------|---------------|--------------------|---|--------------------|
| <b>0001BA</b> | 0 bar to 1 bar     | <b>0100KA</b> | 0 kPa to 100 kPa | <b>0015PA</b> | 0 psi to 15 psi    |   |                    |
| <b>01.6BA</b> | 0 bar to 1.6 bar   | <b>0160KA</b> | 0 kPa to 160 kPa | <b>0025PA</b> | 0 psi to 25 psi    |   |                    |
| <b>02.5BA</b> | 0 bar to 2.5 bar   | <b>0250KA</b> | 0 kPa to 250 kPa | <b>0030PA</b> | 0 psi to 30 psi    |   |                    |
| Gage          |                    | Gage          |                  | Gage          |                    | Gage                                      |                    |
| <b>0060MG</b> | 0 mbar to 60 mbar  | <b>0006KG</b> | 0 kPa to 6 kPa   | <b>0001PG</b> | 0 psi to 1 psi     | <b>0300YG</b>                             | 0 mmHg to 300 mmHg |
| <b>0100MG</b> | 0 mbar to 100 mbar | <b>0010KG</b> | 0 kPa to 10 kPa  | <b>0005PG</b> | 0 psi to 5 psi     |   |                    |
| <b>0160MG</b> | 0 mbar to 160 mbar | <b>0016KG</b> | 0 kPa to 16 kPa  | <b>0015PG</b> | 0 psi to 15 psi    |   |                    |
| <b>0250MG</b> | 0 mbar to 250 mbar | <b>0025KG</b> | 0 kPa to 25 kPa  | <b>0030PG</b> | 0 psi to 30 psi    |   |                    |
| <b>0400MG</b> | 0 bar to 400 mbar  | <b>0040KG</b> | 0 kPa to 40 kPa  |               |                    |   |                    |
| <b>0600MG</b> | 0 bar to 600 mbar  | <b>0060KG</b> | 0 kPa to 60 kPa  |               |                    |   |                    |
| <b>0001BG</b> | 0 bar to 1 bar     | <b>0100KG</b> | 0 kPa to 100 kPa | <b>N</b>      | inH <sub>2</sub> O | Other calibration units may be specified. |                    |
| <b>01.6BG</b> | 0 bar to 1.6 bar   | <b>0160KG</b> | 0 kPa to 160 kPa | <b>G</b>      | MPa                |   |                    |
| <b>02.5BG</b> | 0 bar to 2.5 bar   | <b>0250KG</b> | 0 kPa to 250 kPa | <b>H</b>      | hPa                |   |                    |
|               |                    |               |                  | <b>C</b>      | cmH <sub>2</sub> O |   |                    |

<sup>1</sup> Custom pressure ranges are available. Contact Honeywell Customer Service for more information.

### MPR Series Sensor Mounted on a Breakout Board

Breakout boards, designed for use with the Honeywell SEK002 Sensor Evaluation Kit, are available with the sensor already mounted.

MPR Series with long port mounted on a breakout board.



MPR Series with short port mounted on a breakout board.




TABLE 8. ORDER GUIDE FOR MPR SERIES SENSOR ON BREAKOUT BOARD

| Catalog Listing    | Description  |
|--------------------|--|
| MPRLS0025PA00001AB | Breakout board with 0 psi to 25 psi absolute sensor, long port, with gel, I <sup>2</sup> C = 0x18, transfer function A |
| MPRLS0015PA0000SAB | Breakout board with 0 psi to 15 psi absolute sensor, long port, with gel, SPI, transfer function A                     |
| MPRLS0300YG00001BB | Breakout board with 0 mmHg to 300 mmHg gage sensor, long port, with gel, I <sup>2</sup> C = 0x18, transfer function B  |
| MPRSS0001PG00001CB | Breakout board with 0 psi to 1 psi gage sensor, short port, with gel, I <sup>2</sup> C = 0x18, transfer function C     |

# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS

## MPR SERIES

**TABLE 9. PRESSURE RANGE SPECIFICATIONS FOR 60 MBAR TO 2.5 BAR**

| Pressure Range<br>(See Figure 4.) | Pressure Range    |                   | Unit | Over Pressure <sup>1</sup> | Burst Pressure <sup>2</sup> | Total Error Band After Customer Auto-Zero <sup>3</sup> (%FSS) | Total Error Band, Typical (%FSS) | Transfer Function |
|-----------------------------------|-------------------|-------------------|------|----------------------------|-----------------------------|---|----------------------------------|-------------------|
|                                   | P <sub>MIN.</sub> | P <sub>MAX.</sub> |      |                            |                             |   |                                  |                   |
| <b>Absolute</b>                   |                   |                   |      |                            |                             |   |                                  |                   |
| 0001BA                            | 0                 | 1                 | bar  | 4                          | 8                           | ±1.5 <sup>4</sup>   | ±1.5                             | A, B              |
| 01.6BA                            | 0                 | 1.6               | bar  | 4                          | 8                           | ±1.5 <sup>4</sup>   | ±1.5                             | A, B              |
| 02.5BA                            | 0                 | 2.5               | bar  | 4                          | 8                           | ±1.5 <sup>4</sup>   | ±1.5                             | A, B              |
| <b>Gage</b>                       |                   |                   |      |                            |                             |   |                                  |                   |
| 0060MG                            | 0                 | 60                | mbar | 350                        | 700                         | ±1.25   | ±2.5                             | C                 |
| 0100MG                            | 0                 | 100               | mbar | 350                        | 700                         | ±1.25   | ±2.5                             | C                 |
| 0160MG                            | 0                 | 160               | mbar | 350                        | 700                         | ±1.25   | ±2.5                             | C                 |
| 0250MG                            | 0                 | 250               | mbar | 350                        | 700                         | ±1.25   | ±2.5                             | C                 |
| 0400MG                            | 0                 | 400               | mbar | 4000                       | 8000                        | ±2.0  | ±2.5                             | A, B              |
| 0600MG                            | 0                 | 600               | mbar | 4000                       | 8000                        | ±2.0  | ±2.5                             | A, B              |
| 0001BG                            | 0                 | 1                 | bar  | 4                          | 8                           | ±1.5  | ±2.5                             | A, B              |
| 01.6BG                            | 0                 | 1.6               | bar  | 4                          | 8                           | ±1.5  | ±2.5                             | A, B              |
| 02.5BG                            | 0                 | 2.5               | bar  | 4                          | 8                           | ±1.5  | ±2.5                             | A, B              |

<sup>1</sup> **Overpressure:** The maximum pressure which may safely be applied to the product for it to remain in specification once pressure is returned to the operating pressure range. Exposure to higher pressures may cause permanent damage to the product. Unless otherwise specified this applies to all available pressure ports at any temperature with the operating temperature range. The customer's pressure connection system (tubing or O-rings) must be specified to be equal to, or greater than, the rated overpressure limit. Due to the possibility of light sensitivity, opaque tubing is recommended.

<sup>2</sup> **Burst Pressure:** The maximum pressure that may be applied to any port of the product without causing escape of pressure media. Product should not be expected to function after exposure to any pressure beyond the burst pressure.

<sup>3</sup> **Total Error Band after Customer Auto-Zero:** The maximum deviation from the ideal transfer function over the entire compensated pressure range for a minimum of 24 hours after an auto-zero operation. Includes all errors due to full scale span, pressure non-linearity, pressure hysteresis, and thermal effect on span. Low pressure MPR sensors may exhibit offset shifts after reflow solder. See Technical Note "Auto-Zero Calibration Technique for Pressure Sensors" (008326-1-EN) if this shift is significant in a particular application.

<sup>4</sup> Because atmospheric pressure is continually changing, autozeroing an absolute pressure sensor requires a reference standard. If the actual absolute pressure is important in an application (such as for a barometer), an external precision reference is needed to set the offset to the correct current value of atmospheric pressure. In applications where the difference between multiple absolute sensors is important, any reference may be used (such as one of the other absolute pressure sensors in a system, or even an arbitrary pressure like 14.7 psia), as long as it is consistent and repeatable.



# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS

## MPR SERIES

**TABLE 10. PRESSURE RANGE SPECIFICATIONS FOR 6 KPA TO 250 KPA**

| Pressure Range<br>(See Figure 4.) | Pressure Range    |                   | Unit | Over Pressure <sup>1</sup> | Burst Pressure <sup>2</sup> | Total Error Band After Customer Auto-Zero <sup>3</sup> (%FSS) | Total Error Band, Typical (%FSS) | Transfer Function |
|-----------------------------------|-------------------|-------------------|------|----------------------------|-----------------------------|---|----------------------------------|-------------------|
|                                   | P <sub>MIN.</sub> | P <sub>MAX.</sub> |      |                            |                             |   |                                  |                   |
| <b>Absolute</b>                   |                   |                   |      |                            |                             |   |                                  |                   |
| 0100KA                            | 0                 | 100               | kPa  | 400                        | 800                         | ±1.5 <sup>4</sup>   | ±1.5                             | A, B              |
| 0160KA                            | 0                 | 160               | kPa  | 400                        | 800                         | ±1.5 <sup>4</sup>   | ±1.5                             | A, B              |
| 0250KA                            | 0                 | 250               | kPa  | 400                        | 800                         | ±1.5 <sup>4</sup>   | ±1.5                             | A, B              |
| <b>Gage</b>                       |                   |                   |      |                            |                             |   |                                  |                   |
| 0006KG                            | 0                 | 6                 | kPa  | 35                         | 70                          | ±1.25   | ±2.5                             | C                 |
| 0010KG                            | 0                 | 10                | kPa  | 35                         | 70                          | ±1.25   | ±2.5                             | C                 |
| 0016KG                            | 0                 | 16                | kPa  | 35                         | 70                          | ±1.25   | ±2.5                             | C                 |
| 0025KG                            | 0                 | 25                | kPa  | 35                         | 70                          | ±1.25   | ±2.5                             | C                 |
| 0040KG                            | 0                 | 40                | kPa  | 400                        | 800                         | ±2.0  | ±2.5                             | A, B              |
| 0060KG                            | 0                 | 60                | kPa  | 400                        | 800                         | ±2.0  | ±2.5                             | A, B              |
| 0100KG                            | 0                 | 100               | kPa  | 400                        | 800                         | ±1.5  | ±2.5                             | A, B              |
| 0160KG                            | 0                 | 160               | kPa  | 400                        | 800                         | ±1.5  | ±2.5                             | A, B              |
| 0250KG                            | 0                 | 250               | kPa  | 400                        | 800                         | ±1.5  | ±2.5                             | A, B              |

<sup>1</sup> **Overpressure:** The maximum pressure which may safely be applied to the product for it to remain in specification once pressure is returned to the operating pressure range. Exposure to higher pressures may cause permanent damage to the product. Unless otherwise specified this applies to all available pressure ports at any temperature with the operating temperature range. The customer's pressure connection system (tubing or O-rings) must be specified to be equal to, or greater than, the rated overpressure limit. Due to the possibility of light sensitivity, opaque tubing is recommended.

<sup>2</sup> **Burst Pressure:** The maximum pressure that may be applied to any port of the product without causing escape of pressure media. Product should not be expected to function after exposure to any pressure beyond the burst pressure.

<sup>3</sup> **Total Error Band after Customer Auto-Zero:** The maximum deviation from the ideal transfer function over the entire compensated pressure range for a minimum of 24 hours after an auto-zero operation. Includes all errors due to full scale span, pressure non-linearity, pressure hysteresis, and thermal effect on span. Low pressure MPR sensors may exhibit offset shifts after reflow solder. See Technical Note "Auto-Zero Calibration Technique for Pressure Sensors" (008326-1-EN) if this shift is significant in a particular application.

<sup>4</sup> Because atmospheric pressure is continually changing, autozeroing an absolute pressure sensor requires a reference standard. If the actual absolute pressure is important in an application (such as for a barometer), an external precision reference is needed to set the offset to the correct current value of atmospheric pressure. In applications where the difference between multiple absolute sensors is important, any reference may be used (such as one of the other absolute pressure sensors in a system, or even an arbitrary pressure like 14.7 psia), as long as it is consistent and repeatable.

# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS

## MPR SERIES

**TABLE 11. PRESSURE RANGE SPECIFICATIONS FOR 1 PSI TO 30 PSI**

| Pressure Range<br>(See Figure 4.) | Pressure Range    |                   | Unit | Over Pressure <sup>1</sup> | Burst Pressure <sup>2</sup> | Total Error Band After Customer Auto-Zero <sup>3</sup> (%FSS) | Total Error Band, Typical (%FSS) | Transfer Function |
|-----------------------------------|-------------------|-------------------|------|----------------------------|-----------------------------|---|----------------------------------|-------------------|
|                                   | P <sub>MIN.</sub> | P <sub>MAX.</sub> |      |                            |                             |   |                                  |                   |
| <b>Absolute</b>                   |                   |                   |      |                            |                             |   |                                  |                   |
| 0015PA                            | 0                 | 15                | psi  | 60                         | 120                         | ±1.5 <sup>4</sup>   | ±1.5                             | A, B              |
| 0025PA                            | 0                 | 25                | psi  | 60                         | 120                         | ±1.5 <sup>4</sup>   | ±1.5                             | A, B              |
| 0030PA                            | 0                 | 30                | psi  | 60                         | 120                         | ±1.5 <sup>4</sup>   | ±1.5                             | A, B              |
| <b>Gage</b>                       |                   |                   |      |                            |                             |   |                                  |                   |
| 0001PG                            | 0                 | 1                 | psi  | 5                          | 10                          | ±1.25   | ±2.5                             | C                 |
| 0005PG                            | 0                 | 5                 | psi  | 60                         | 120                         | ±2.0  | ±2.5                             | A, B              |
| 0015PG                            | 0                 | 15                | psi  | 60                         | 120                         | ±1.5  | ±2.5                             | A, B              |
| 0030PG                            | 0                 | 30                | psi  | 60                         | 120                         | ±1.5  | ±2.5                             | A, B              |

<sup>1</sup>**Overpressure:** The maximum pressure which may safely be applied to the product for it to remain in specification once pressure is returned to the operating pressure range. Exposure to higher pressures may cause permanent damage to the product. Unless otherwise specified this applies to all available pressure ports at any temperature with the operating temperature range. The customer's pressure connection system (tubing or O-rings) must be specified to be equal to, or greater than, the rated overpressure limit. Due to the possibility of light sensitivity, opaque tubing is recommended.

<sup>2</sup>**Burst Pressure:** The maximum pressure that may be applied to any port of the product without causing escape of pressure media. Product should not be expected to function after exposure to any pressure beyond the burst pressure.

<sup>3</sup>**Total Error Band after Customer Auto-Zero:** The maximum deviation from the ideal transfer function over the entire compensated pressure range for a minimum of 24 hours after an auto-zero operation. Includes all errors due to full scale span, pressure non-linearity, pressure hysteresis, and thermal effect on span. Low pressure MPR sensors may exhibit offset shifts after reflow solder. See Technical Note "Auto-Zero Calibration Technique for Pressure Sensors" (008326-1-EN) if this shift is significant in a particular application.

<sup>4</sup>Because atmospheric pressure is continually changing, autozeroing an absolute pressure sensor requires a reference standard. If the actual absolute pressure is important in an application (such as for a barometer), an external precision reference is needed to set the offset to the correct current value of atmospheric pressure. In applications where the difference between multiple absolute sensors is important, any reference may be used (such as one of the other absolute pressure sensors in a system, or even an arbitrary pressure like 14.7 psia), as long as it is consistent and repeatable.

**TABLE 12. PRESSURE RANGE SPECIFICATIONS FOR 0 MMHG TO 300 MMHG**

| Pressure Range<br>(See Figure 4.) | Pressure Range    |                   | Unit | Over Pressure <sup>1</sup> | Burst Pressure <sup>2</sup> | Total Error Band After Customer Auto-Zero <sup>3</sup> (%FSS) | Total Error Band, Typical (%FSS) | Transfer Function |
|-----------------------------------|-------------------|-------------------|------|----------------------------|-----------------------------|---|----------------------------------|-------------------|
|                                   | P <sub>MIN.</sub> | P <sub>MAX.</sub> |      |                            |                             |   |                                  |                   |
| <b>Gage</b>                       |                   |                   |      |                            |                             |   |                                  |                   |
| 0300YG                            | 0                 | 300               | mmHg | 3100                       | 6200                        | ±2.0  | ±2.5                             | B                 |

<sup>1</sup>**Overpressure:** The maximum pressure which may safely be applied to the product for it to remain in specification once pressure is returned to the operating pressure range. Exposure to higher pressures may cause permanent damage to the product. Unless otherwise specified this applies to all available pressure ports at any temperature with the operating temperature range. The customer's pressure connection system (tubing or O-rings) must be specified to be equal to, or greater than, the rated overpressure limit. Due to the possibility of light sensitivity, opaque tubing is recommended.

<sup>2</sup>**Burst Pressure:** The maximum pressure that may be applied to any port of the product without causing escape of pressure media. Product should not be expected to function after exposure to any pressure beyond the burst pressure.

<sup>3</sup>**Total Error Band after Customer Auto-Zero:** The maximum deviation from the ideal transfer function over the entire compensated pressure range for a minimum of 24 hours after an auto-zero operation. Includes all errors due to full scale span, pressure non-linearity, pressure hysteresis, and thermal effect on span. Low pressure MPR sensors may exhibit offset shifts after reflow solder. See Technical Note "Auto-Zero Calibration Technique for Pressure Sensors" (008326-1-EN) if this shift is significant in a particular application.


# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

## 1.0 GENERAL INFORMATION

Please see pages 19-22 for product dimensions, pinouts, tape and reel dimensions, Recommended Pick and Place Geometry, and recommended tubing.

## 2.0 PINOUT AND FUNCTIONALITY (SEE TABLE 13.)

**TABLE 13. PINOUT AND FUNCTIONALITY**



| Pad Number | Name            | Description  |
|------------|-----------------|--|
| 1          | SS              | Sensor Select: Chip select for SPI sensor  |
| 2          | MOSI/SDA        | Master Out Sensor In: Data in for SPI sensor; data in/out for I <sup>2</sup> C sensor  |
| 3          | SCLK/SCL        | Clock input for SPI and I <sup>2</sup> C sensor  |
| 4          | VO+             | V <sub>OUT+</sub> pin in piezoresistive Wheatstone Bridge: Anti-aliasing filter can be connected between VO+ and VO-   |
| 5          | NC              | No connection  |
| 6          | VO-             | V <sub>OUT-</sub> pin in piezoresistive Wheatstone Bridge: Anti-aliasing filter can be connected between VO- and VO+   |
| 7          | MISO            | Master In Sensor Out: Data output for SPI sensor   |
| 8          | EOC             | End-of-conversion indicator: This pin is set high when a measurement and calculation have been completed and the data is ready to be clocked out   |
| 9          | RES             | Reset: This pin can be connected and used to control safe resetting of the sensor. RES is active-low; a V <sub>DD</sub> -V <sub>SS</sub> -V <sub>DD</sub> transition at the RES pin leads to a complete sensor reset |
| 10         | V <sub>SS</sub> | Ground reference voltage signal  |
| 11         | NC              | No connection  |
| 12         | V <sub>DD</sub> | Positive supply voltage  |

## 3.0 START-UP TIMING

On power-up, the MPR Series sensor is able to receive the first command after 1 ms from when the V<sub>DD</sub> supply is within operating specifications. The MPR Series sensor can begin the first measurement after 2.5 ms from when the V<sub>DD</sub> supply is operational. Alternatively, instead of a power-on reset, a reset and new power-up sequence can be triggered by an IC-reset signal (high low) at the RES pin.

## 4.0 POWER SUPPLY REQUIREMENT

Verify that system power to the sensor meets the V<sub>DD</sub> rising slope requirement (minimum V<sub>DD</sub> rising slope is at least 10 V/ms). If not, use the RES pin to bring the sensor out of reset once the system power has stabilized.

# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

## 5.0 REFERENCE CIRCUIT DESIGN

### 5.1 I<sup>2</sup>C AND SPI CIRCUIT DIAGRAMS (SEE FIGURES 5 AND 6.)

FIGURE 5. I<sup>2</sup>C CIRCUIT DIAGRAM





FIGURE 6. SPI CIRCUIT DIAGRAM



### 5.2 BYPASS CAPACITOR USE

## NOTICE

Ensure bypass capacitors are integrated into the end user design to ensure output noise suppression.

# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

## 6.0 I<sup>2</sup>C COMMUNICATIONS


### 6.1 I<sup>2</sup>C BUS CONFIGURATION (SEE FIGURE 7.)

The I<sup>2</sup>C bus is a simple, serial 8-bit oriented computer bus for efficient I<sup>2</sup>C (Inter-IC) control. It provides good support for communication between different ICs across short circuit-board distances, such as interfacing microcontrollers with various low speed peripheral devices. For detailed specifications of the I<sup>2</sup>C protocol, see Rev. 6 (April 2014) of the I<sup>2</sup>C Bus Specification (source: NXP Semiconductor at <https://www.nxp.com/docs/en/user-guide/UM10204.pdf>).

Each device connected to the bus is software addressable by a unique address and a simple Master/Sensor relationship that exists at all times. The output stages of devices connected to the bus are designed around an open collector architecture. Because of this, pull-up resistors to +V<sub>DD</sub> must be provided on the bus. Both SDA and SCL are bidirectional lines, and it is important to system performance to match the capacitive loads on both lines. In addition, in accordance with the I<sup>2</sup>C specification, the maximum allowable capacitance on either line is 400 pF to ensure reliable edge transitions at 400 kHz clock speeds.

When the bus is free, both lines are pulled up to +V<sub>DD</sub>. Data on the I<sup>2</sup>C bus can be transferred at a rate up to 100 kbit/s in the standard-mode, or up to 400 kbit/s in the fast-mode.

**FIGURE 7. I<sup>2</sup>C BUS CONFIGURATION**



### 6.2 I<sup>2</sup>C DATA TRANSFER

The MPR Series I<sup>2</sup>C Sensors will only respond to requests from a Master device. Following the address and read bit from the Master, the MPR Series Sensors are designed to output up to 4 bytes of data. The first data byte is the Status Byte (8-bit) and the second to fourth bytes are the compensated pressure output (24-bit).

### 6.3 I<sup>2</sup>C SENSOR ADDRESS

Each MPR Series I<sup>2</sup>C Sensor is referenced on the bus by a 7-bit sensor address. The default address for the MPR Series is 24 (0x18). Other available standard addresses are: 08 (0x08), 40 (0x28), 56 (0x38), 72 (0x48), 88 (0x58), 104 (0x68), 120 (0x78). (Other custom values are available. Please contact Honeywell Customer Service with questions regarding custom Sensor addresses.)

### 6.4 I<sup>2</sup>C PRESSURE READING

To read out a compensated pressure reading, the Master generates a START condition and sends the Sensor address followed by a read bit (1). After the Sensor generates an acknowledge, it will transmit up to 4 bytes of data. The first data byte is the Status Byte (8-bit) and the second to fourth bytes are the compensated pressure output (24-bit). The Master must acknowledge the receipt of each byte, and can terminate the communication by sending a Not Acknowledge (NACK) bit followed by a Stop bit after receiving the required bytes of data.

# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

## 6.5 I<sup>2</sup>C STATUS BYTE (SEE TABLE 14.)

| TABLE 14. I <sup>2</sup> C STATUS BYTE EXPLANATION |  |   |
|--|--|---|
| Bit (Meaning)                                      | Status   | Comment   |
| 7  | always 0   | —   |
| 6 (Power indication)                               | 1 = device is powered<br>0 = device is not powered     | Needed for the SPI Mode where the Master reads all zeroes if the device is not powered or in power-on reset (POR).                                  |
| 5 (Busy flag)                                      | 1 = device is busy                                     | Indicates that the data for the last command is not yet available. No new commands are processed if the device is busy.                             |
| 4  | always 0   | —   |
| 3  | always 0   | —   |
| 2 (Memory integrity/error flag)                    | 0 = integrity test passed<br>1 = integrity test failed | Indicates whether the checksum-based integrity check passed or failed; the memory error status bit is calculated only during the power-up sequence. |
| 1  | always 0   | —   |
| 0 (Math saturation)                                | 1 = internal math saturation has occurred              | —   |

## 6.6 I<sup>2</sup>C COMMUNICATIONS

### 6.6.1 I<sup>2</sup>C Output Measurement Command

To communicate with the MPR Series I<sup>2</sup>C output sensor using an Output Measurement Command of “0xAA”, followed by “0x00” “0x00”, follow the steps shown in Table 15. This command will cause the device to exit Standby Mode and enter Operating Mode. At the conclusion of the measurement cycle, the device will automatically re-enter Standby Mode.

| TABLE 15. I <sup>2</sup> C OUTPUT MEASUREMENT COMMAND |  |   |
|---|--|---|
| Step  | Action   | Notes   |
| 1   | <p>7-bit<br/>Write bit</p>   | <p>Master to Sensor<br/>Sensor to Master</p>  |
| 2   | <p><b>Option 1:</b> Wait until the busy flag in the Status Byte clears.</p> <p><b>Option 2:</b> Wait for at least 5 ms for the data conversion to occur.</p> <p><b>Option 3:</b> Wait for the EOC indicator.</p> <p>7-bit<br/>Read bit</p> | <p>S Start condition<br/>P Stop condition<br/>A Acknowledge<br/>N Not acknowledge</p> |
| 3   | <p>To read the 24-bit pressure output along with the 8-bit Status Byte:</p> <p>7-bit<br/>Read bit</p>  |   |

# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

## 6.6.2 I<sup>2</sup>C Sensor Address of 0x18


To communicate with the MPR Series I<sup>2</sup>C output sensor with an I<sup>2</sup>C Sensor Address of 0x18 (hex), follow the steps shown in Table 16.

**TABLE 16. I<sup>2</sup>C SENSOR ADDRESS OF 0X18 COMMUNICATIONS**

| Step | Action   | Notes   |
|------|--|---|
| 1    |  | <ul style="list-style-type: none"> <li><span style="display: inline-block; width: 10px; height: 10px; background-color: #d9ead3; border: 1px solid #000; margin-right: 5px;"></span> Master to Sensor</li> <li><span style="display: inline-block; width: 10px; height: 10px; background-color: #d9ead3; border: 1px solid #000; margin-right: 5px;"></span> Sensor to Master</li> <li><span style="display: inline-block; width: 10px; height: 10px; background-color: #d9ead3; border: 1px solid #000; margin-right: 5px;"></span> Start condition</li> <li><span style="display: inline-block; width: 10px; height: 10px; background-color: #d9ead3; border: 1px solid #000; margin-right: 5px;"></span> Stop condition</li> <li><span style="display: inline-block; width: 10px; height: 10px; background-color: #d9ead3; border: 1px solid #000; margin-right: 5px;"></span> Acknowledge</li> <li><span style="display: inline-block; width: 10px; height: 10px; background-color: #d9ead3; border: 1px solid #000; margin-right: 5px;"></span> Not acknowledge</li> </ul> |
| 2    | <p><b>Option 1:</b> Wait until the busy flag in the Status Byte clears.</p> <p><b>Option 2:</b> Wait for at least 5 ms for the data conversion to occur.</p> <p><b>Option 3:</b> Wait for the EOC indicator.</p> |   |
| 3    | <p>To read the 24-bit pressure output along with the 8-bit Status Byte:</p>  |   |

## 6.7 I<sup>2</sup>C TIMING AND LEVEL PARAMETERS (SEE TABLE 17.)

**TABLE 17. I<sup>2</sup>C BUS TIMING DIAGRAM AND PARAMETERS**



| Characteristic   | Abbreviation | Min. | Typ. | Max. | Unit         |
|--|--------------|------|------|------|--------------|
| SCLK clock frequency                                     | $f_{SCL}$    | 100  | —    | 400  | kHz          |
| Start condition hold time relative to SCL edge           | $t_{HDSTA}$  | 0.1  | —    | —    | $\mu$ s      |
| Minimum SCLK clock low width <sup>1</sup>                | $t_{LOW}$    | 0.6  | —    | —    | $\mu$ s      |
| Minimum SCLK clock high width <sup>1</sup>               | $t_{HIGH}$   | 0.6  | —    | —    | $\mu$ s      |
| Start condition setup time relative to SCL edge          | $t_{SUSTA}$  | 0.1  | —    | —    | $\mu$ s      |
| Data hold time on SDA relative to SCL edge               | $t_{HDDAT}$  | 0    | —    | —    | $\mu$ s      |
| Data setup time on SDA relative to SCL edge              | $t_{SUDAT}$  | 0.1  | —    | —    | $\mu$ s      |
| Stop condition setup time on SCL                         | $t_{SUSTO}$  | 0.1  | —    | —    | $\mu$ s      |
| Bus free time between stop condition and start condition | $t_{BUS}$    | 2    | —    | —    | $\mu$ s      |
| Output level low   | $Out_{low}$  | —    | 0    | 0.2  | $V_{DD}$     |
| Output level high  | $Out_{high}$ | 0.8  | 1    | —    | $V_{DD}$     |
| Pull-up resistance on SDA and SCL                        | $R_p$        | 1    | —    | 50   | k $\Omega$ m |

<sup>1</sup>Combined low and high widths must equal or exceed minimum SCLK period.

# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

## 6.8 REFERENCE CODE (ARDUINO/GENUINO UNO) FOR I<sup>2</sup>C INTERFACE

See also Section 8.0 for details and examples of MPR Series Pressure and Temperature output calculations.

```
#include<Arduino.h>
#include<Wire.h>

uint8_t id = 0x28; // i2c address
uint8_t data[7]; // holds output data
uint8_t cmd[3] = {0xAA, 0x00, 0x00}; // command to be sent
double press_counts = 0; // digital pressure reading [counts]
double temp_counts = 0; // digital temperature reading [counts]
double pressure = 0; // pressure reading [bar, psi, kPa, etc.]
double temperature = 0; // temperature reading in deg C
double outputmax = 15099494; // output at maximum pressure [counts]
double outputmin = 1677722; // output at minimum pressure [counts]
double pmax = 1; // maximum value of pressure range [bar, psi, kPa, etc.]
double pmin = 0; // minimum value of pressure range [bar, psi, kPa, etc.]
double percentage = 0; // holds percentage of full scale data
char printBuffer[200], cBuff[20], percBuff[20], pBuff[20], tBuff[20];
void setup() {
  Serial.begin(9600);
  while (!Serial) {
    delay(10);
  }
  Wire.begin();
  sprintf(printBuffer, "\nStatus Register, 24 - bit Sensor data, Digital Pressure Counts,\
  Percentage of full scale pressure, Pressure Output, Temperature\n");
  Serial.println(printBuffer);
}
void loop() {
  Wire.beginTransmission(id);
  int stat = Wire.write (cmd, 3); // write command to the sensor
  stat |= Wire.endTransmission();
  delay(10);
  Wire.requestFrom(id, 7); // read back Sensor data 7 bytes
  int i = 0;
  for (i = 0; i < 7; i++) {
    data [i] = Wire.read();
  }
  press_counts = data[3] + data[2] * 256 + data[1] * 65536; // calculate digital pressure counts
  temp_counts = data[6] + data[5] * 256 + data[4] * 65536; // calculate digital temperature counts
  temperature = (temp_counts * 200 / 16777215) - 50; // calculate temperature in deg c
  percentage = (press_counts / 16777215) * 100; // calculate pressure as percentage of full scale
  //calculation of pressure value according to equation 2 of datasheet
  pressure = ((press_counts - outputmin) * (pmax - pmin)) / (outputmax - outputmin) + pmin;
  dtostrf(press_counts, 4, 1, cBuff);
  dtostrf(percentage, 4, 3, percBuff);
  dtostrf(pressure, 4, 3, pBuff);
  dtostrf(temperature, 4, 3, tBuff);
  /*
  The below code prints the raw data as well as the processed data
  Data format : Status Register, 24-bit Sensor Data, Digital Counts, percentage of full scale
  pressure,
  pressure output, temperature
  */
  sprintf(printBuffer, " %x\t% 2x % 2x % 2x\t% s\t% s\t% s\t% s \n", data[0], data[1], data[2],
  data[3],
  cBuff, percBuff, pBuff, tBuff);
  Serial.print(printBuffer);
  delay(10);
}
```




# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

## 7.0 SPI COMMUNICATIONS

### 7.1 SPI DEFINITION

The Serial Peripheral Interface (SPI) is a simple bus system for synchronous serial communication between one Master and one or more Sensors. It operates either in full-duplex or half-duplex mode, allowing communication to occur in either both directions simultaneously, or in one direction only. The Master device initiates an information transfer on the bus and generates clock and control signals. Sensors are controlled by the Master through individual Sensor Select (SS) lines and are active only when selected. The MPR Series SPI sensors operate in full-duplex mode only, with data transfer from the Sensor to the Master. This data transmission uses four, unidirectional bus lines. The Master controls SCLK, MOSI and SS; the Sensor controls MISO. (See Figure 8.)


**FIGURE 8. SPI BUS CONFIGURATION**

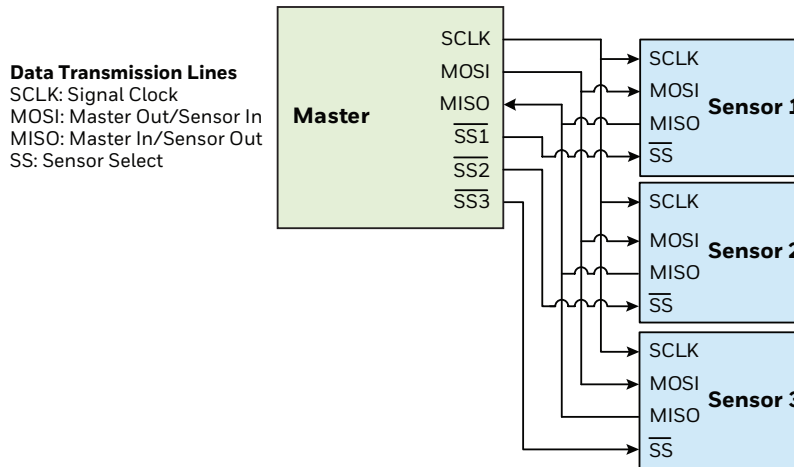

### 7.2 SPI DATA TRANSFER

Start communication with the MPR Series SPI sensors by de-asserting the Sensor Select (SS) line. At this point, the sensor is no longer idle, and will begin sending data once a clock is received. MPR Series SPI sensors are configured for SPI operation in mode 0 (clock polarity is 0 and clock phase is 0). (See Figure 9.)

**FIGURE 9. EXAMPLE OF 1 BYTE SPI DATA TRANSFER**



Once the clocking begins, the MPR Series SPI sensor is designed to output up to 4 bytes of data. The first data byte is the Status Byte (8-bit) and the second to fourth bytes are the compensated pressure output (24-bit).

### 7.3 SPI PRESSURE READING

To read out a compensated pressure reading, the Master generates the necessary clock signal after activating the sensor with the Sensor Select (SS) line. The sensor will transmit up to 4 bytes of data. The first data byte is the Status Byte (8-bit) and the second to fourth bytes are the compensated pressure output (24-bit). The Master can terminate the communication by stopping the clock and deactivating the SS line.

### 7.4 SPI STATUS BYTE

The SPI status byte contains the bits shown in Table 18.

# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

## 7.5 SPI COMMUNICATION


To communicate with the MPR Series SPI output sensor using an Output Measurement Command of “0xAA”, followed by “0x00” “0x00”, follow the steps shown in Table 18. This command will cause the device to exit Standby Mode and enter Operating Mode. At the conclusion of the measurement cycle, the device will automatically re-enter Standby Mode.

**TABLE 18. SPI OUTPUT MEASUREMENT COMMAND**

| Step | Action  |                        |                   |                   | Notes  |
|------|---|------------------------|-------------------|-------------------|--|
| 1    | The data on MISO depend on the preceding command. Discard the data on the MISO line.  |                        |                   |                   |  |
|      | MOSI  | 0xAA                   | 0x00              | 0x00              | <div style="display: flex; flex-direction: column; align-items: center;"> <div style="width: 15px; height: 15px; background-color: #d9ead3; border: 1px solid #ccc; margin-bottom: 5px;"></div> Master to Sensor           <div style="width: 15px; height: 15px; background-color: #d9ead3; border: 1px solid #ccc; margin-bottom: 5px;"></div> Sensor to Master         </div> |
|      |   | Command other than NOP | CmdData <15:8>    | CmdData <7:0>     |  |
| MISO | Status  | Data                   | Data              |                   |  |
| 2    | <b>Option 1:</b> Wait until the busy flag in the Status Byte clears.<br><b>Option 2:</b> Wait for at least 5 ms for the data conversion to occur.<br><b>Option 3:</b> Wait for the EOC indicator. |                        |                   |                   | <ul style="list-style-type: none"> <li>NOP Command is “0xF0”.</li> </ul>   |
|      | MOSI  | 0xF0                   | Command = NOP     |                   |  |
|      |   | MISO                   | Status            |                   |  |
| 3    | To read the 24-bit pressure output along with the 8-bit Status Byte:  |                        |                   |                   |  |
|      | MOSI  | 0xF0                   | 0x00              | 0x00              | 0x00   |
|      |   | Command = NOP          | 00 <sub>Hex</sub> | 00 <sub>Hex</sub> | 00 <sub>Hex</sub>  |
| MISO | Status  | SensorDat <24:16>      | SensorDat <15:8>  | SensorDat <7:0>   |  |

## 7.6 SPI TIMING AND LEVEL PARAMETERS (SEE TABLE 19.)

**TABLE 19. SPI BUS TIMING DIAGRAM AND PARAMETERS**



| Characteristic                             | Abbreviation | Min. | Typ. | Max. | Unit     |
|--|--------------|------|------|------|----------|
| SCLK clock frequency                       | $f_{SCL}$    | 50   | —    | 800  | kHz      |
| SS drop to first clock edge                | $t_{HDSS}$   | 2.5  | —    | —    | $\mu$ S  |
| Minimum SCLK clock low width <sup>1</sup>  | $t_{LOW}$    | 0.6  | —    | —    | $\mu$ S  |
| Minimum SCLK clock high width <sup>1</sup> | $t_{HIGH}$   | 0.6  | —    | —    | $\mu$ S  |
| Clock edge to data transition              | $t_{CLKD}$   | 0    | —    | —    | $\mu$ S  |
| Rise of SS relative to last clock edge     | $t_{SUSS}$   | 0.1  | —    | —    | $\mu$ S  |
| Bus free time between rise and fall of SS  | $t_{BUS}$    | 2    | —    | —    | $\mu$ S  |
| Output level low                           | $Out_{low}$  | —    | 0    | 0.2  | $V_{DD}$ |
| Output level high                          | $Out_{high}$ | 0.8  | 1    | —    | $V_{DD}$ |

<sup>1</sup>Combined low and high widths must equal or exceed minimum SCLK period.

# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

## 7.7 REFERENCE CODE (ARDUINO/GENUINO UNO) FOR SPI INTERFACE

See also Section 8.0 for details and examples of MPR Series Pressure and Temperature output calculations.

```
#include<Arduino.h>
#include<SPI.h>

double press_counts = 0; // digital pressure reading [counts]
double temp_counts = 0; // digital temperature reading [counts]
double pressure = 0; // pressure reading [bar, psi, kPa, etc.]
double temperature = 0; // temperature reading in deg C
double outputmax = 15099494; // output at maximum pressure [counts]
double outputmin = 1677722; // output at minimum pressure [counts]
double pmax = 1; // maximum value of pressure range [bar, psi, kPa, etc.]
double pmin = 0; // minimum value of pressure range [bar, psi, kPa, etc.]
double percentage = 0; // holds percentage of full scale data
char printBuffer[200], cBuff[20], percBuff[20], pBuff[20], tBuff[20];
void setup() {
  Serial.begin(9600);
  while (!Serial) {
    delay(10);
  }
  sprintf(printBuffer, "\nStatus Register, 24-bit Sensor data, Digital Pressure Counts,\
Percentage of full scale pressure,Pressure Output, Temperature\n");
  Serial.println(printBuffer);
  SPI.begin();
  pinMode(10, OUTPUT); // pin 10 as SS
  digitalWrite(10, HIGH); // set SS High
}
void loop() {
  delay(1);
  while (1) {
    uint8_t data[7] = {0xFA, 0x00, 0x00, 0x00, 0x00, 0x00, 0x00}; // holds output data
    uint8_t cmd[3] = {0xAA, 0x00, 0x00}; // command to be sent
    SPI.beginTransaction(SPISettings(200000, MSBFIRST, SPI_MODE0)); //SPI at 200kHz
    digitalWrite(10, LOW); // set SS Low
    SPI.transfer(cmd, 3); // send Read Command
    digitalWrite(10, HIGH); // set SS High
    delay(10); // wait for conversion
    digitalWrite(10, LOW);
    SPI.transfer(data, 7);
    digitalWrite(10, HIGH);
    SPI.endTransaction();
    press_counts = data[3] + data[2] * 256 + data[1] * 65536; // calculate digital pressure counts
    temp_counts = data[6] + data[5] * 256 + data[4] * 65536; // calculate digital temperature counts
    temperature = (temp_counts * 200 / 16777215) - 50; // calculate temperature in deg c
    percentage = (press_counts / 16777215) * 100; // calculate pressure as percentage of full scale
    //calculation of pressure value according to equation 2 of datasheet
    pressure = ((press_counts - outputmin) * (pmax - pmin)) / (outputmax - outputmin) + pmin;
    dtostrf(press_counts, 4, 1, cBuff);
    dtostrf(percentage, 4, 3, percBuff);
    dtostrf(pressure, 4, 3, pBuff);
    dtostrf(temperature, 4, 3, tBuff);
    /*
     The below code prints the raw data as well as the processed data
     Data format : Status Register, 24-bit Sensor Data, Digital Counts, percentage of full scale
     pressure, pressure output,
     temperature
    */
    sprintf(printBuffer, "%x\t%2x %2x %2x\t%s\t%s\t%s\t%s \n", data[0], data[1], data[2], data[3],
      cBuff, percBuff, pBuff, tBuff);
    Serial.print(printBuffer);
    delay(10);
  }
}
```

# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

## 8.0 MPR SERIES SENSOR OUTPUT PRESSURE CALCULATION

The MPR Series sensor output can be expressed by the transfer function of the device as shown in Equation 1:

### Equation 1: Pressure Sensor Transfer Function

$$\text{Output} = \frac{\text{Output}_{\text{max.}} - \text{Output}_{\text{min.}}}{P_{\text{max.}} - P_{\text{min.}}} * (\text{Pressure} - P_{\text{min.}}) + \text{Output}_{\text{min.}}$$

Rearranging this equation to solve for Pressure, we get Equation 2:

### Equation 2: Pressure Output Function

$$\text{Pressure} = \frac{(\text{Output} - \text{Output}_{\text{min.}}) * (P_{\text{max.}} - P_{\text{min.}})}{\text{Output}_{\text{max.}} - \text{Output}_{\text{min.}}} + P_{\text{min.}}$$

Where:

Output<sub>max.</sub> = output at maximum pressure [counts]

Output<sub>min.</sub> = output at minimum pressure [counts]

P<sub>max.</sub> = maximum value of pressure range [bar, psi, kPa, etc.]

P<sub>min.</sub> = minimum value of pressure range [bar, psi, kPa, etc.]

Pressure = pressure reading [bar, psi, kPa, etc.]

Output = digital pressure reading [counts]

**Example:** Calculate the pressure for a -1 psi to 1 psi gage sensor with a 10% to 90% calibration, and a pressure output of 14260634 (decimal) counts:

Output<sub>max.</sub> = 15099494 counts (90% of 2<sup>24</sup> counts or 0xE66666)

Output<sub>min.</sub> = 1677722 counts (10% of 2<sup>24</sup> counts or 0x19999A)

P<sub>max.</sub> = 1 psi

P<sub>min.</sub> = -1 psi

Pressure = pressure in psi

Output = 14260634 counts

$$\text{Pressure} = \left[ \frac{(14260634 - 1677722) * (1 - (-1))}{15099494 - 1677722} \right] + (-1)$$


$$\text{Pressure} = \frac{25165824}{13421772} + (-1)$$

$$\text{Pressure} = 0.875 \text{ psi}$$


# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

FIGURE 10. LONG PORT AND RECOMMENDED PCB PAD LAYOUT DIMENSIONS (FOR REFERENCE ONLY: MM [IN.]

## Sensor




## Recommended PCB pad layout




# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

FIGURE 11. SHORT PORT AND RECOMMENDED PCB PAD LAYOUT DIMENSIONS (FOR REFERENCE ONLY: MM [IN.] )


## Sensor



## Reflowable protective silicone cap




## Recommended PCB pad layout




# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

FIGURE 12. TAPE AND REEL DIMENSIONS (FOR REFERENCE ONLY: MM.)


## Long Port Tape



## Short Port Tape



## Reel



# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

## REFLOWABLE PROTECTIVE SILICONE CAP

Every short port MPR Series sensor is shipped with a reflowable protective silicone cap intended to protect the sensor's protective gel throughout the assembly process (see Figure 10). This cap can withstand lead-free, reflow temperatures and is intended to be removed after the end-user has completed assembly of the MPR sensor to the mating assembly.

## REFLOWABLE PROTECTIVE SILICONE CAP REMOVAL

Removal of the cap may easily be done manually using ESD-safe tweezers; however, if possible, and to eliminate possible sensor protective gel damage, the cap removal process should be done in a semi-automated or automated manner. If the cap must be removed manually, follow this removal process:

- Using ESD-safe tweezers, grasp the silicone cap midway up the straight port and lift the cap up vertically until it is no longer supported by the sensor housing.
- At this point, stop the vertical movement and relieve the grasp of the tweezers.
- Regrasp the cap in the unsupported area and continue the vertical movement until the cap is free and clear of the sensor's protective gel.
- Ensure that the sensor's protective gel is not damaged during the cap removal process.

## RECOMMENDED TUBING

See Table 20 for recommended tubing information.

## RECOMMENDED O-RINGS

For O-Ring location, size and recommended part numbers, see the following:

- Short port sensor: Figure 13 and Table 21.
- Long port sensor: Figure 14 and Table 22.

**TABLE 20. RECOMMENDED TUBING**

| Manufacturer      | Type                      | Part Number | ID (in) | OD (in) | Pressure at 25°C (psi) |
|-------------------|---------------------------|-------------|---------|---------|------------------------|
| Frelin-Wade       | Fre-Thane® (polyurethane) | 1A-156-11   | 0.093   | 0.156   | 210                    |
| Frelin-Wade       | nylon                     | 1A-200-01   | 0.093   | 0.125   | 270                    |
| NewAge Industries | PVC                       | 1100225     | 0.094   | 0.156   | 42                     |
| NewAge Industries | silicone                  | 2800315     | 0.094   | 0.156   | 20                     |



# MICROPRESSURE BOARD MOUNT PRESSURE SENSORS MPR SERIES

FIGURE 13. RECOMMENDED MANIFOLD DESIGN FOR SHORT PORT SENSOR WITH O-RING




TABLE 21. RECOMMENDED O-RINGS FOR SHORT PORT SENSOR

| ID (mm) | Cross Section (Width) (mm) | Supplier | Part Number | Material               | Hardness      |
|---------|----------------------------|----------|-------------|------------------------|---------------|
| 4.00    | 2.00                       | McMaster | 9262K163    | Buna-N                 | Durometer 70A |
| 4.00    | 2.00                       | McMaster | 1174N421    | Buna-N                 | Durometer 50A |
| 4.00    | 2.00                       | McMaster | 1185N82     | Viton® Fluoroelastomer | Durometer 75A |
| 4.00    | 2.00                       | McMaster | 9263K163    | Viton® Fluoroelastomer | Durometer 75A |
| 4.00    | 2.00                       | McMaster | 5233T47     | silicone               | Durometer 70A |
| 4.00    | 2.00                       | McMaster | 1295N222    | Viton® Fluoroelastomer | Durometer 75A |
| 4.00    | 2.00                       | McMaster | 1278N15     | Kalrez 4079            | Durometer 75A |

FIGURE 14. RECOMMENDED MANIFOLD DESIGN FOR LONG PORT SENSOR WITH O-RING




TABLE 22. RECOMMENDED O-RINGS FOR LONG PORT SENSOR

| ID (mm) | Cross Section (Width) (mm) | Supplier | Part Number | Material               | Hardness      |
|---------|----------------------------|----------|-------------|------------------------|---------------|
| 2.20    | 1.60                       | McMaster | 9262K131    | Buna-N                 | Durometer 70A |
| 2.20    | 1.60                       | McMaster | 9263K131    | Viton® Fluoroelastomer | Durometer 75A |
| 2.20    | 1.60                       | McMaster | 5233T142    | silicone               | Durometer 70A |